



Assessment performed
Apr 18, 2026 · 11:34

CERVICAL ASSESSMENT RECORD

John Smith

PATIENT IDENTIFIER

SAMPLE · 0001

CLINICIAN

Hugo Park · Chiropractor · AHPRA CHI0002895435

PRACTICE

DeskNeck · 309 George Street, Sydney

DESKNECK ASSESSMENT RECORD

SAMPLE DOCUMENT — NOT FOR CLINICAL USE



OVERVIEW

Spine health profile

Four domains, measured separately. Each is scored on its own and compared to people your age. Read them together. There is no single grade.

MOBILITY · ROM

● MIXED

76/100

range of motion



How far the neck moves. Most directions sit in range. Left lateral flexion is the clear outlier.

POSITION SENSE · JPE

● STRONG

84/100

joint position error



How accurately the head returns to neutral with eyes closed. Strong. Rotation is the cleanest.

SENSORIMOTOR CONTROL

● WATCH

64/100

target tracking



How well movement tracks a moving target. Fine when slow. Drifts as speed increases.

SYMPTOM LOAD

● LOW

16/72

self-reported



Self-reported total. Low overall. Cognitive items carry nearly all of the weight.

Colour shows where a result sits against age-matched norms — **within range**, **monitor**, or **below range**. It is a starting point for re-testing, not a verdict.



SELF-REPORT

Symptoms

What's present, and how much it interferes. Rated 0 to 6. Zero is absent. Six is hard to function. This tracks change over time — not cause.

DURATION OF CURRENT SYMPTOMS

Acute or subacute

NO

Chronic

NO

HISTORY RELATED TO CURRENT SYMPTOMS

Head impact / concussion

NO

Idiopathic neck pain

YES

Traumatic neck pain

NO

Degenerative neck pain

NO

PHYSICAL

Balance problems

0

Dizziness

0

Headache

0

Jaw pain or dysfunction

1

Neck pain

1

Visual disturbances

0

EMOTIONAL

Anxiety

0

Depression

0

COGNITIVE

Difficulty concentrating

5

Difficulty remembering

5

Feeling in a fog

3

SLEEP

Sleep disturbance

1

TOTAL SYMPTOM LOAD

16 / 72




OBJECTIVE · VALD HUMANTRAK

Range of motion

76

SCORE


Maximum movement of the cervical spine, in degrees, across six directions. The outer ring is the age-matched norm; the inner arc is what was achieved.

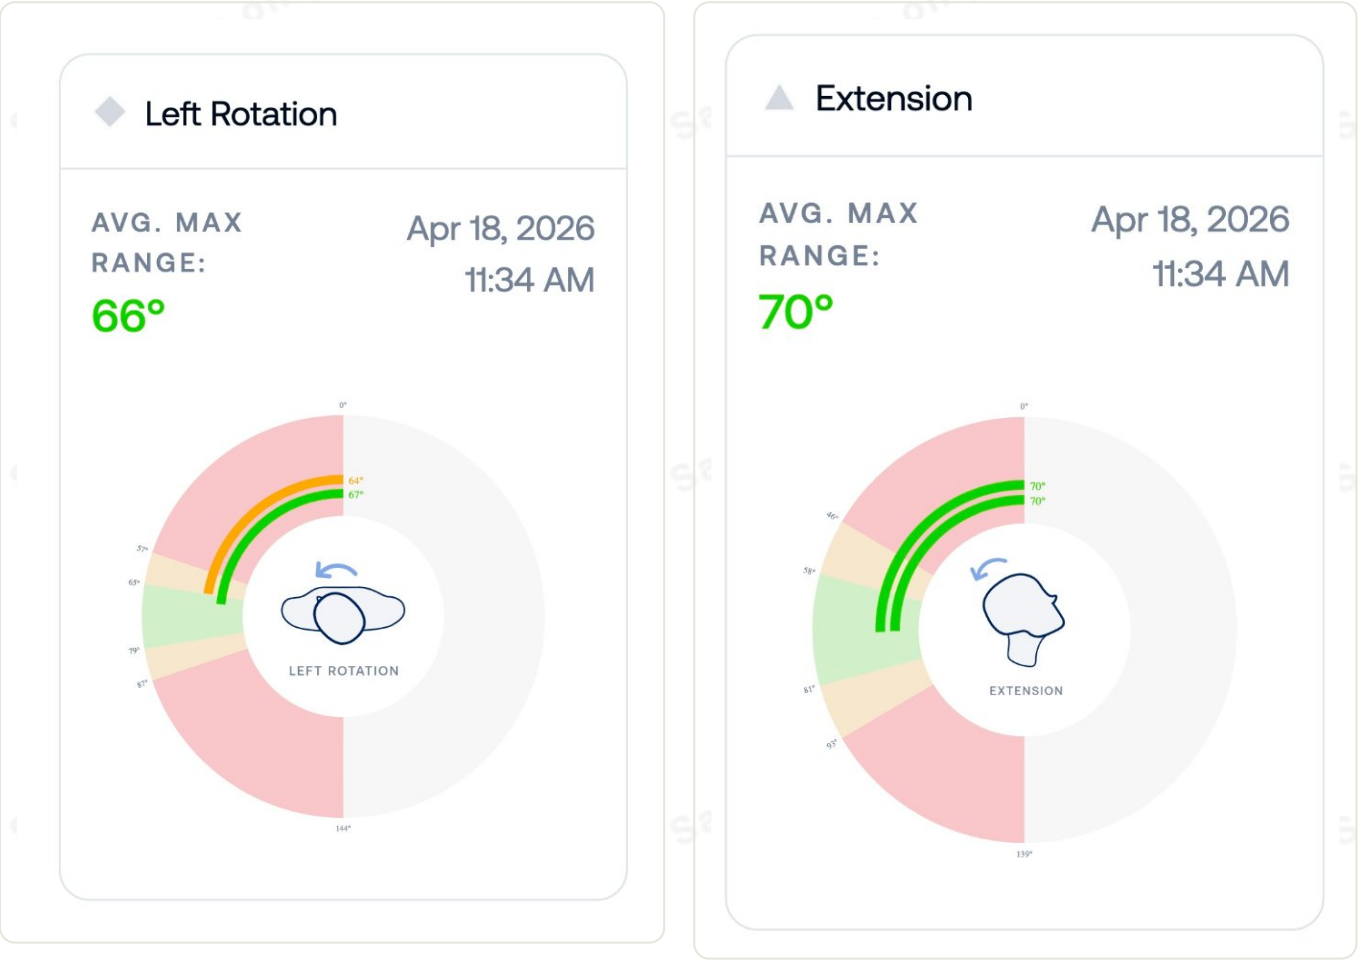

■ Right Rotation

AVG. MAX
RANGE:


57°

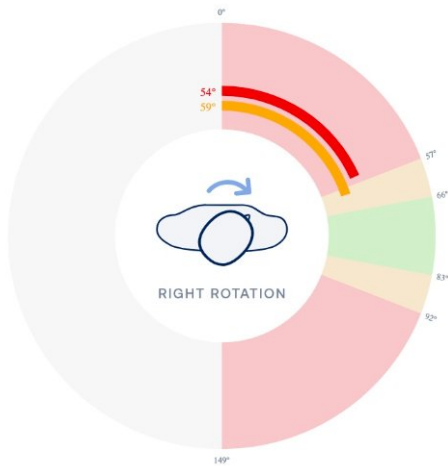Apr 18, 2026
11:34 AM

+ Left Lateral Flexion

AVG. MAX
RANGE:


25°

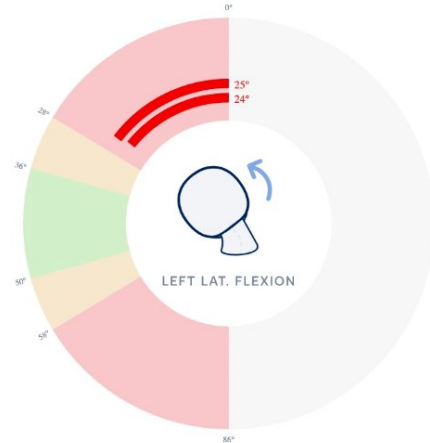Apr 18, 2026
11:34 AM

▼ Flexion

AVG. MAX
RANGE:


49°

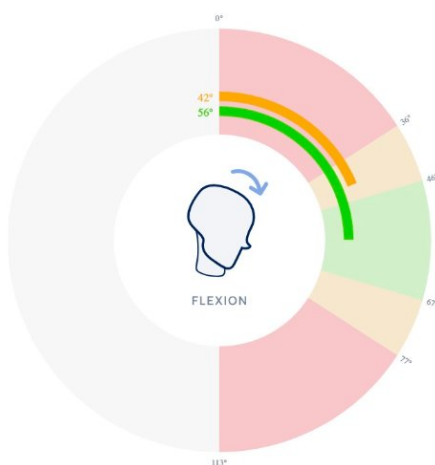Apr 18, 2026
11:34 AM

× Right Lateral Flexion

AVG. MAX
RANGE:

37°

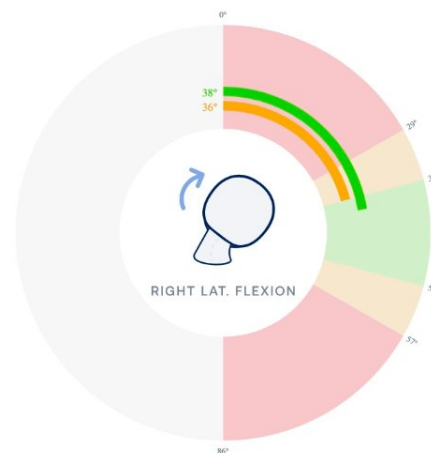Apr 18, 2026
11:34 AM



NUMERICAL RESULTS

Range of motion — values

Average maximum range per direction, in degrees.

Left rotation

AVERAGE

MAX RANGE

66°

Extension

AVERAGE

MAX RANGE

70°

Right rotation

AVERAGE

MAX RANGE

57°

Left lat. flexion

AVERAGE

MAX RANGE

25°

Flexion

AVERAGE

MAX RANGE

49°

Right lat. flexion

AVERAGE


MAX RANGE

37°


OBJECTIVE · MOVEMENT QUALITY

Accessory movement


A clean movement happens in one plane. These plots show what the neck did in the other two planes while performing each primary direction. Lines that hold the centre band are clean. Lines drifting to the edges are compensation. Two repetitions shown.

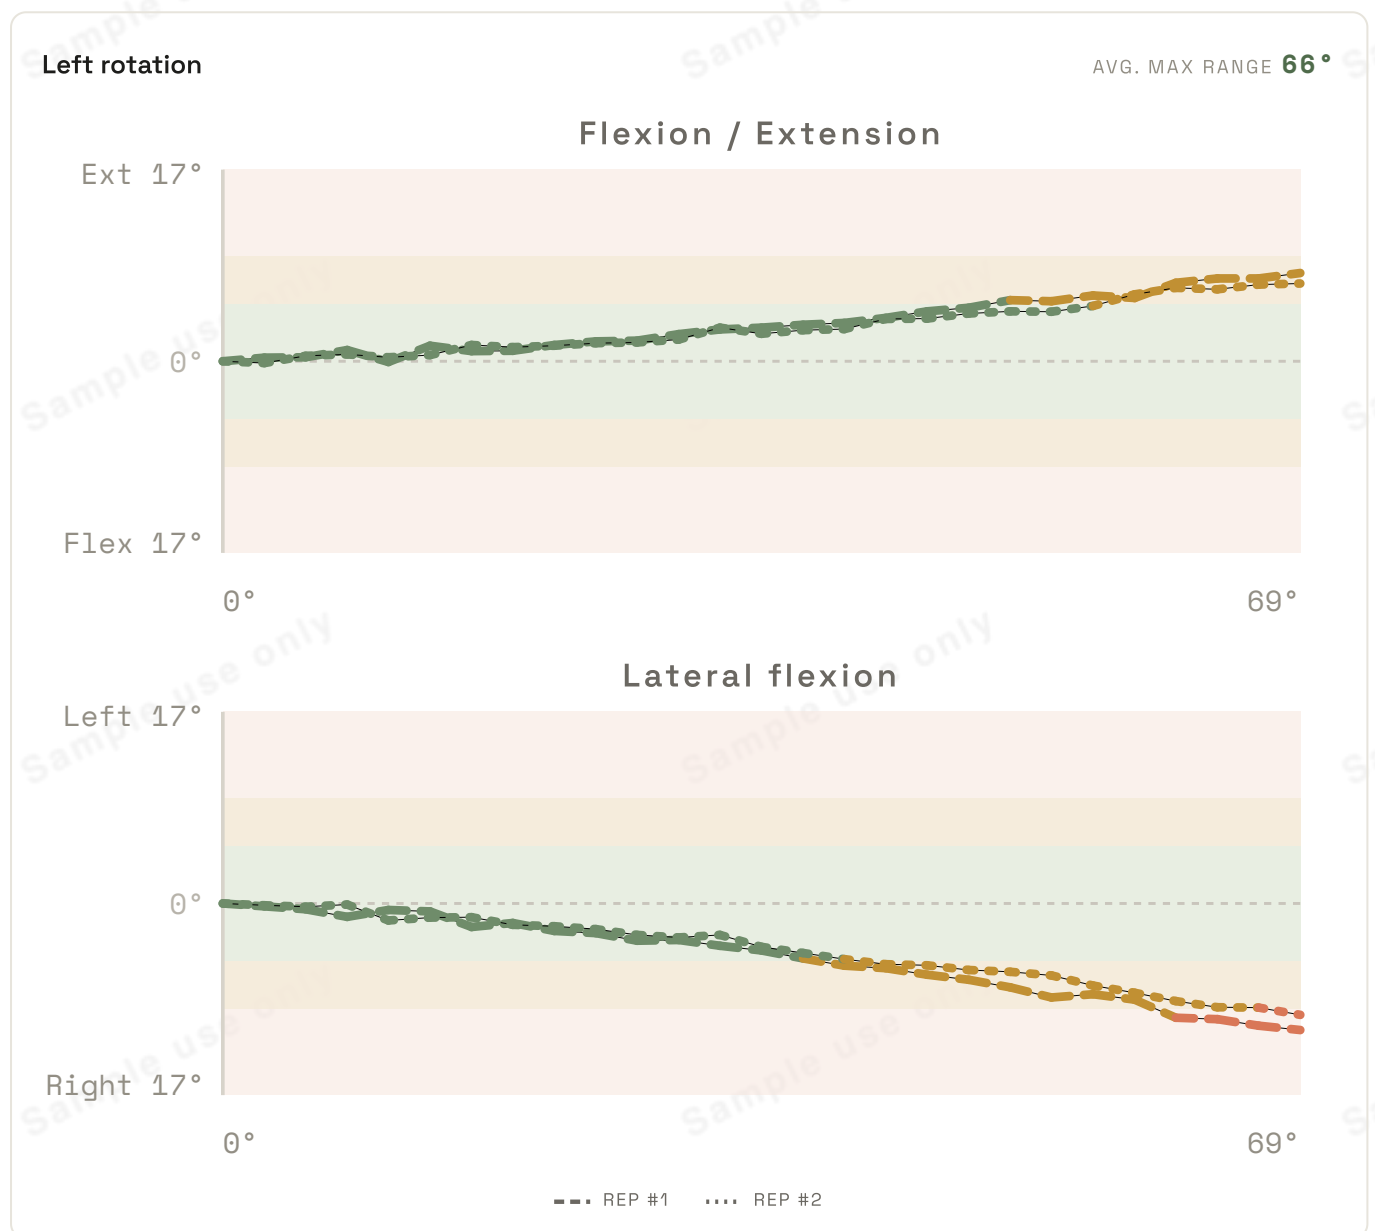

Flexion / Extension

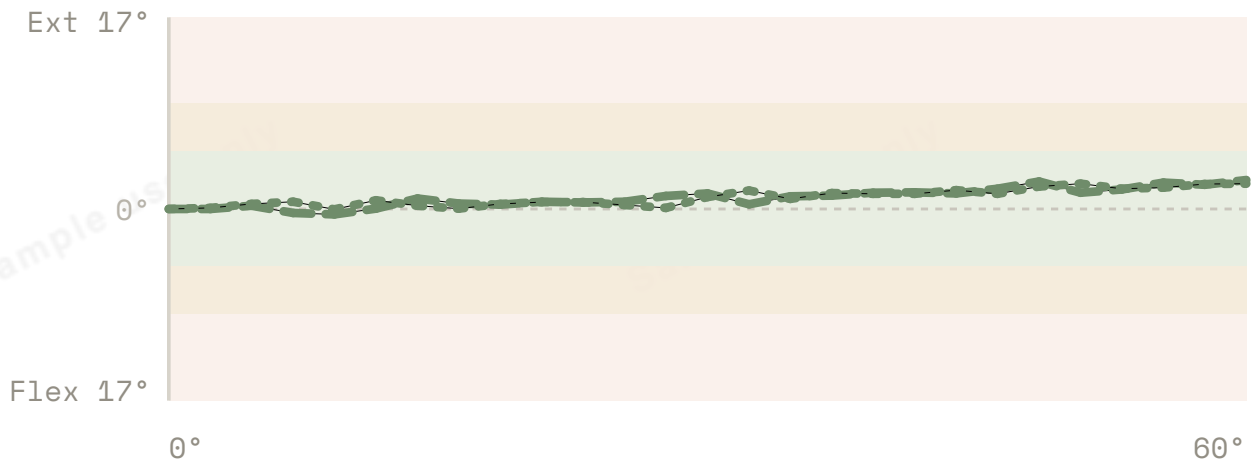


Lateral flexion


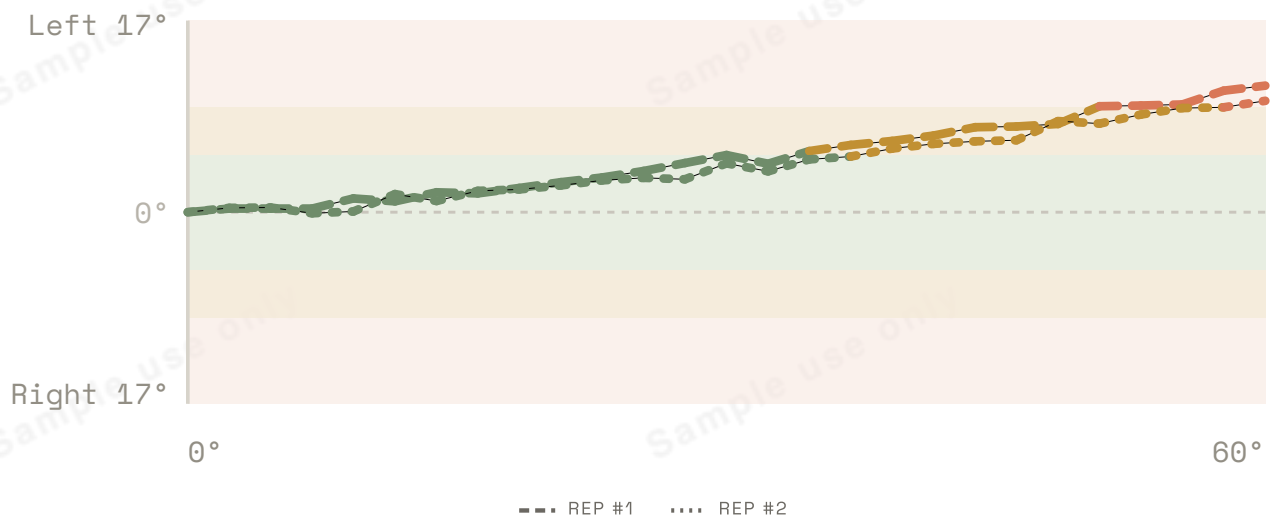


Extension

AVG. MAX RANGE 70°

Rotation

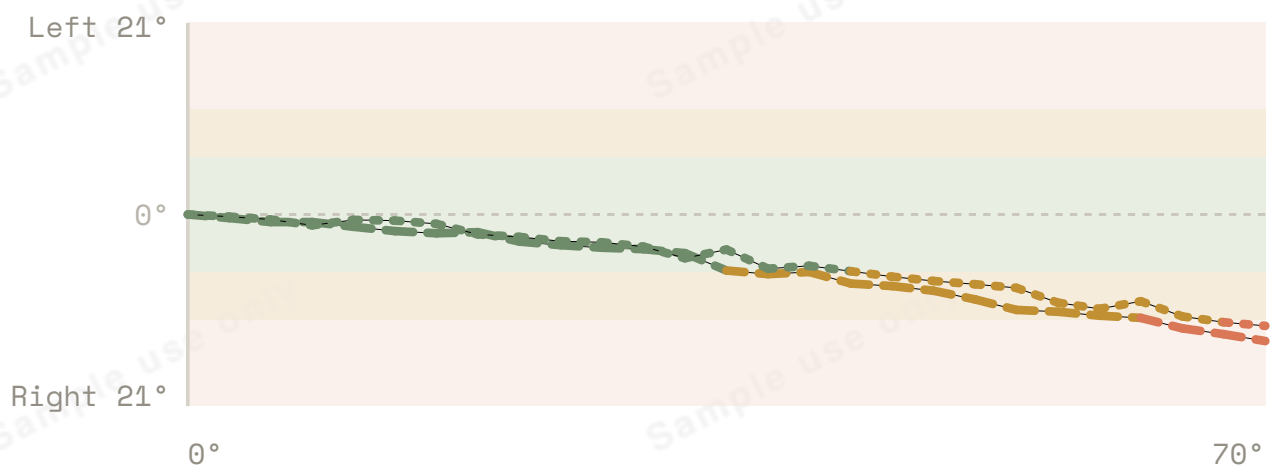

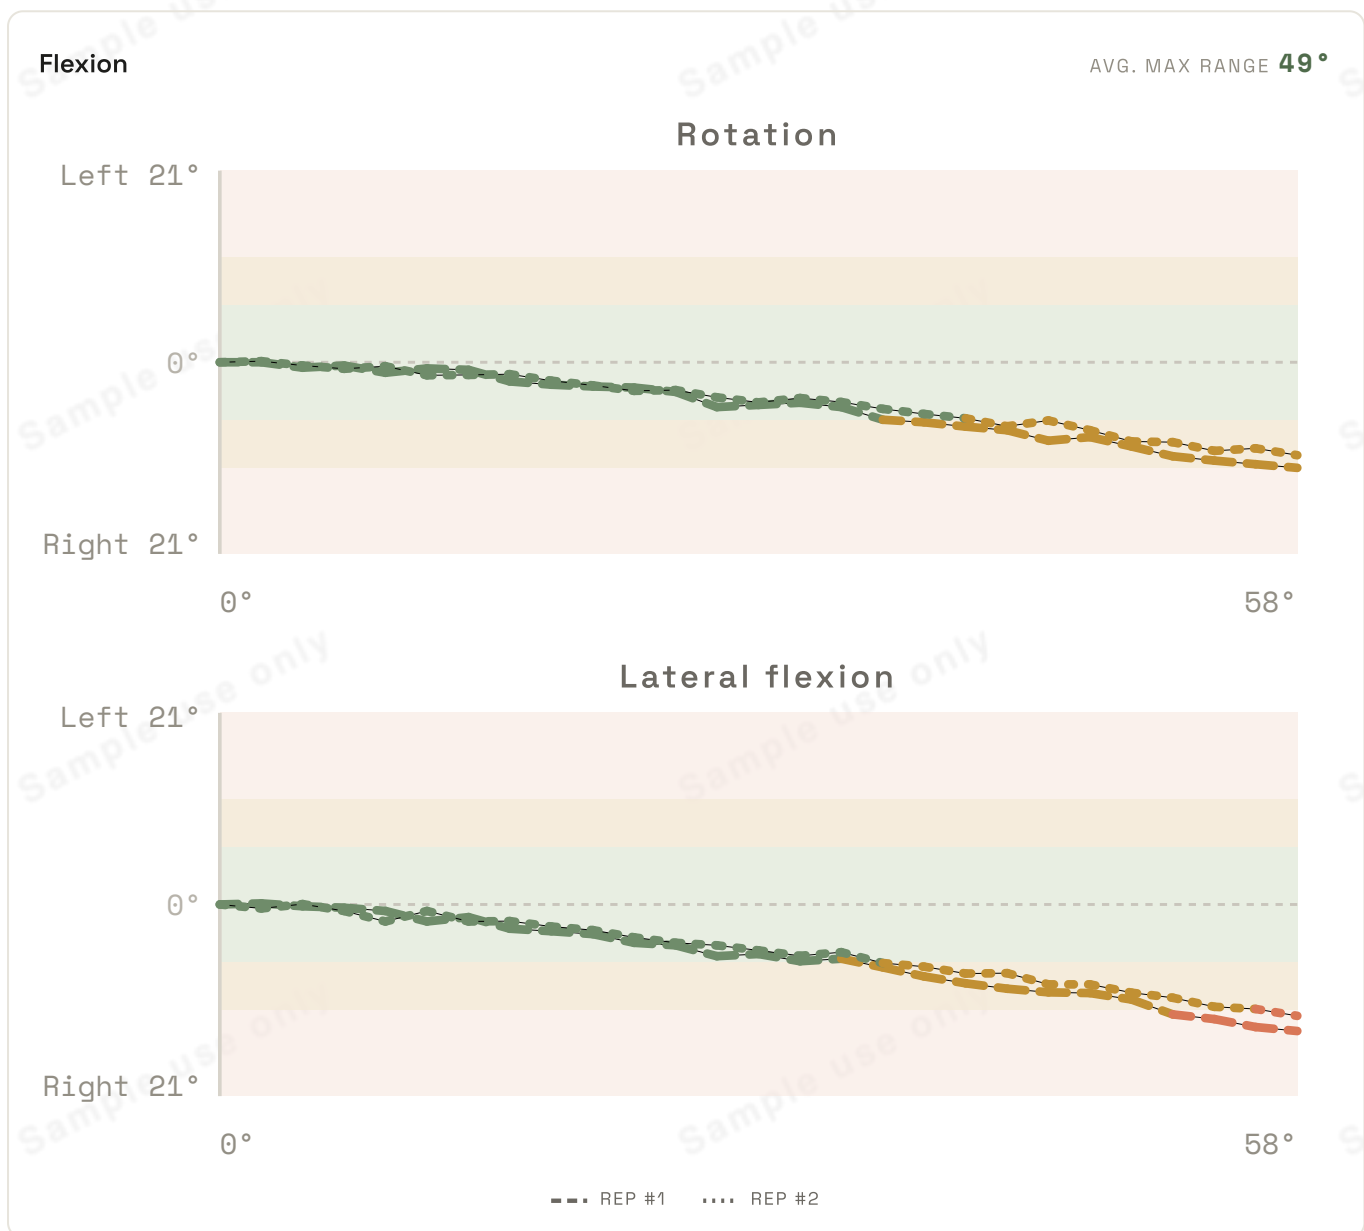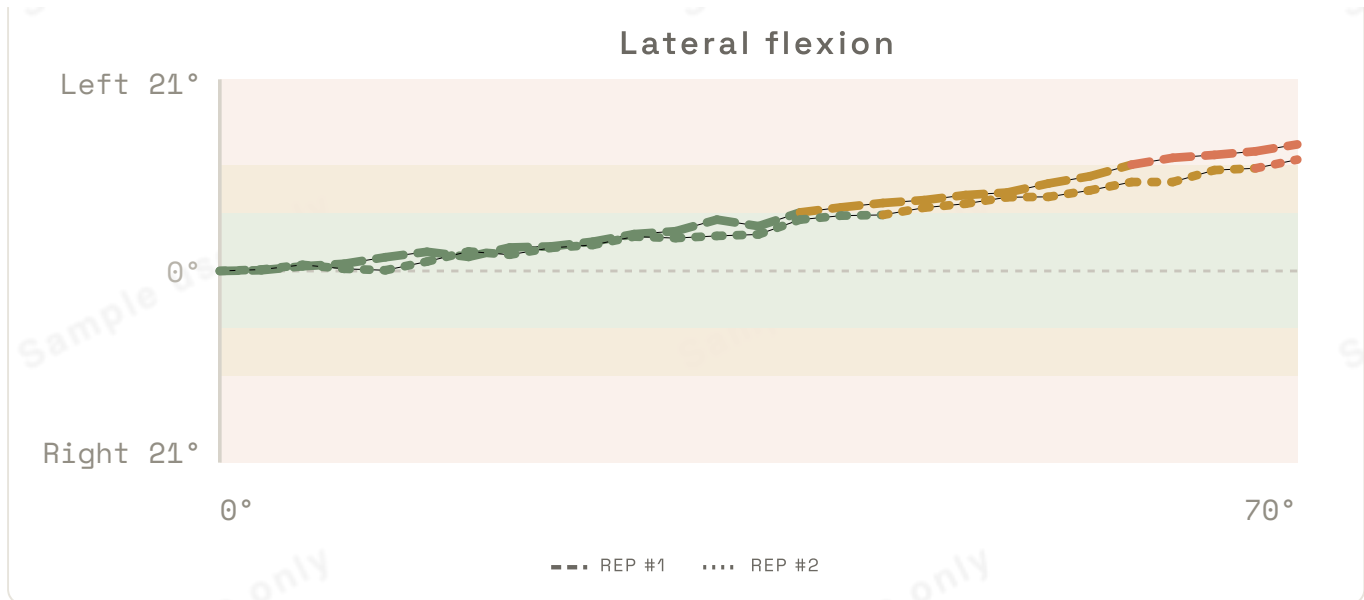




John Smith · SAMPLE 0001


Apr 18, 2026

OBJECTIVE · MOVEMENT QUALITY

Accessory movement — lateral flexion

Coupled motion during left and right lateral flexion.

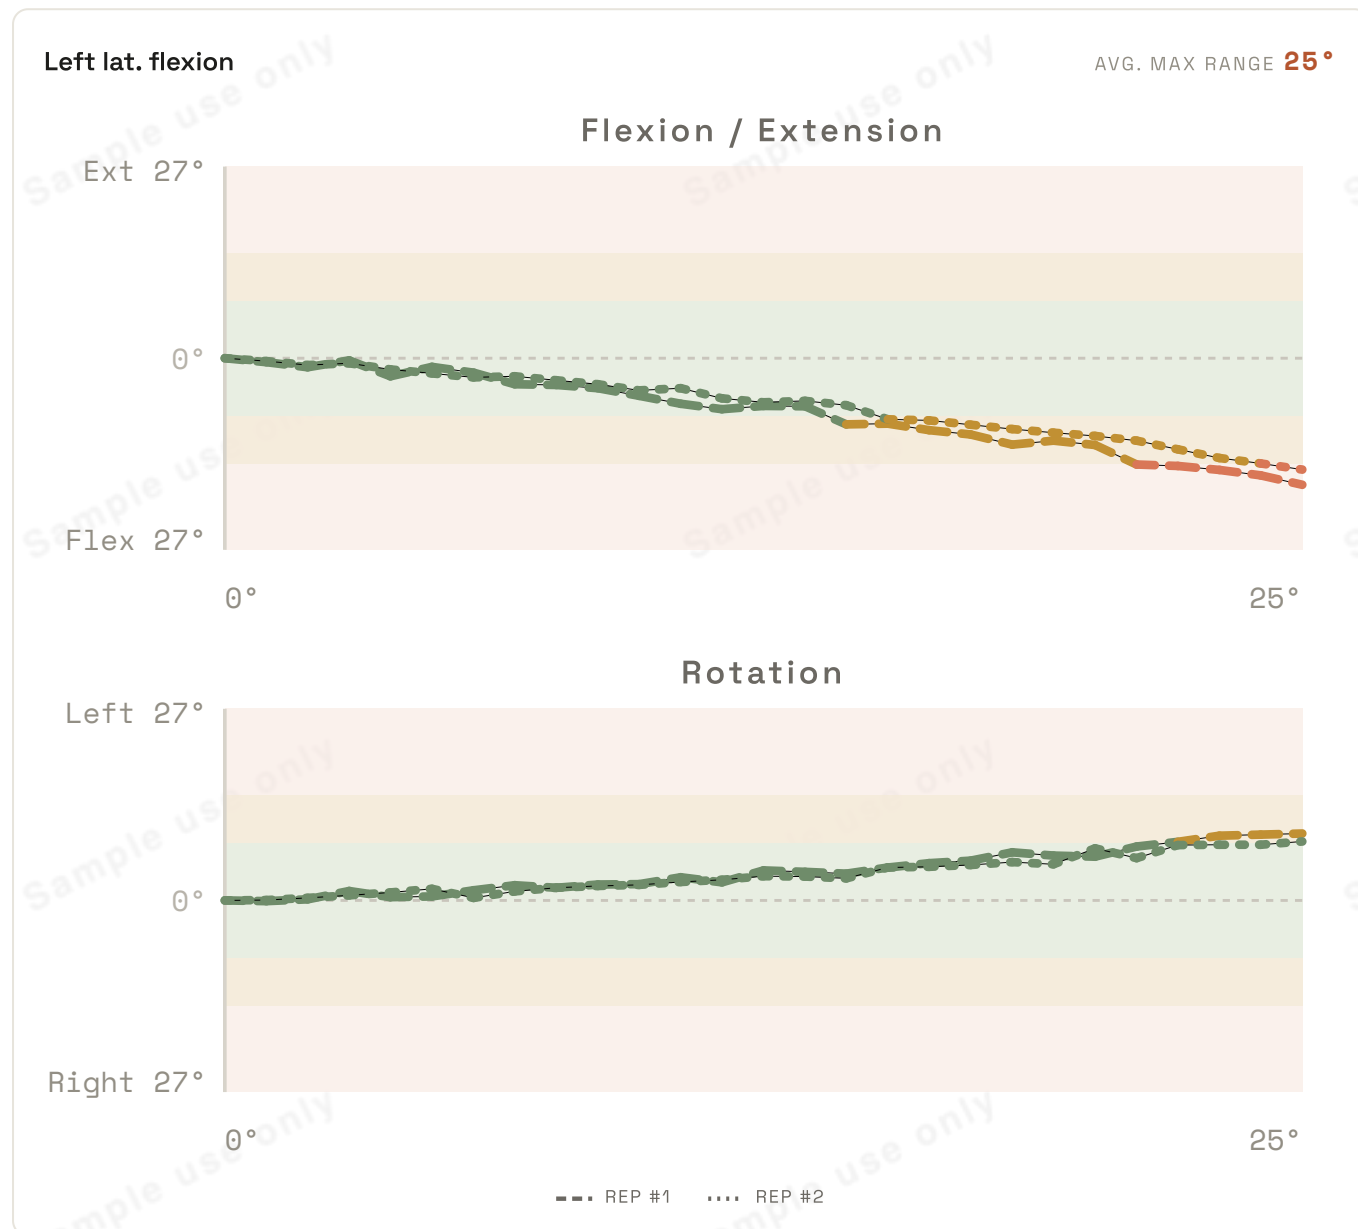**Right lat. flexion**AVG. MAX RANGE **37°**

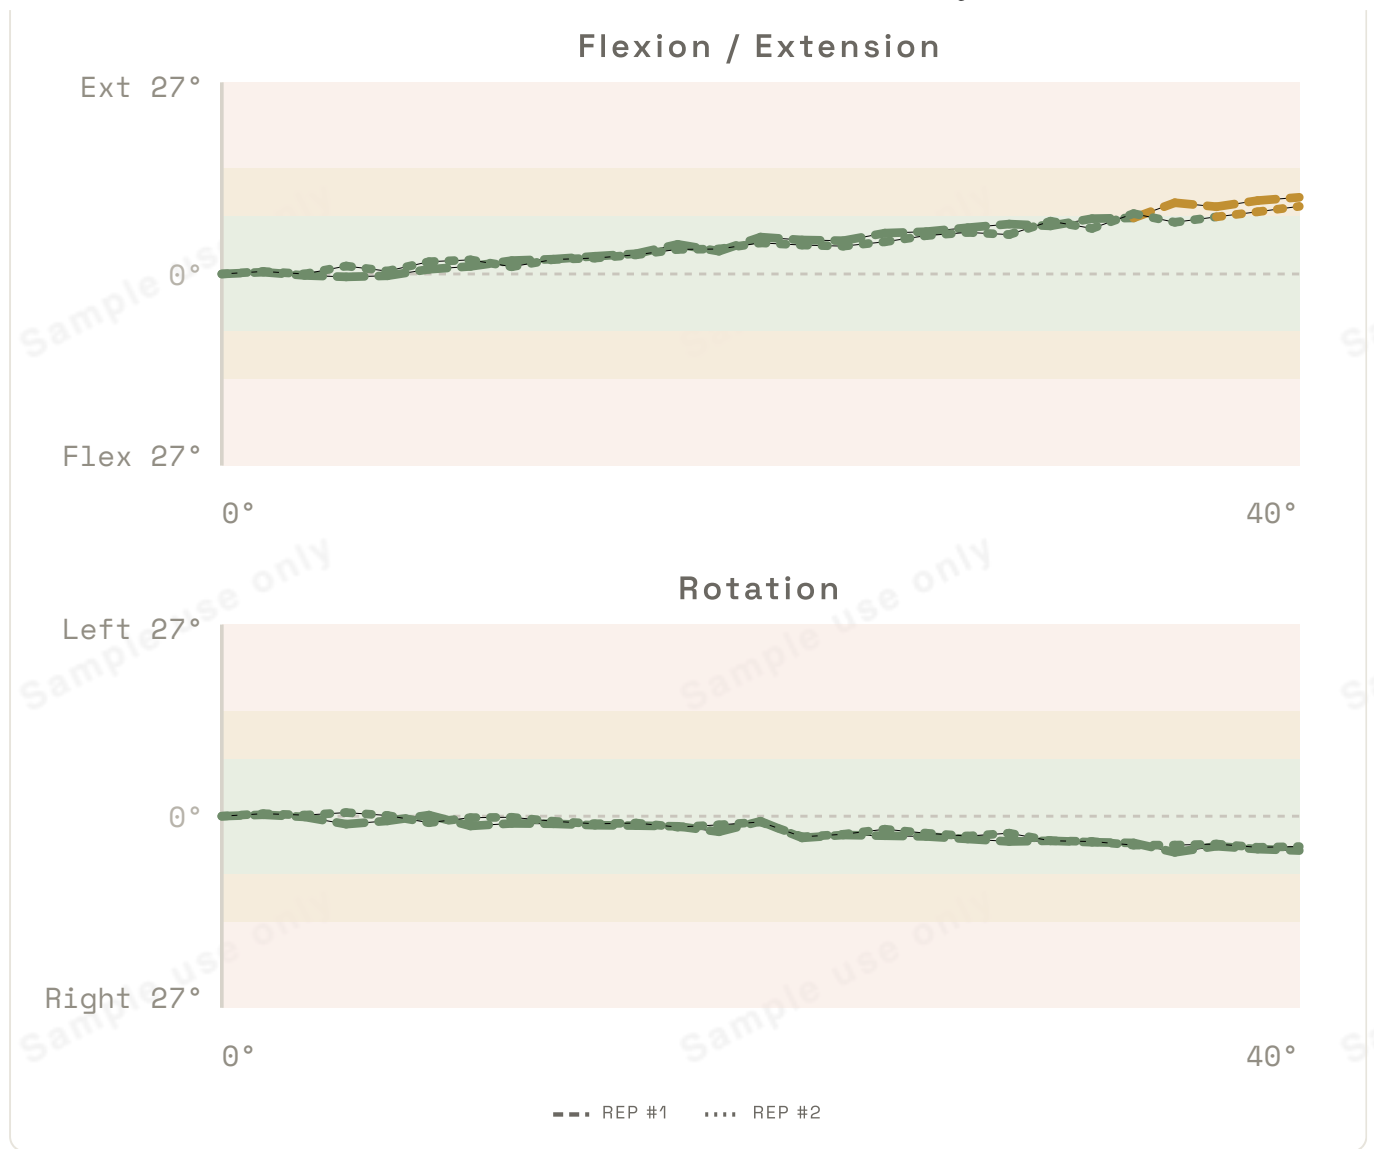

Compensation isn't failure — it's information. It shows where the system borrows from neighbouring planes, and gives the re-test something specific to move.







OBJECTIVE · PROPRIOCEPTION

Joint position error

84
SCORE

Eyes closed, the patient moves, then returns to neutral. The gap between where they land and true neutral is the error, in degrees. Lower is better.

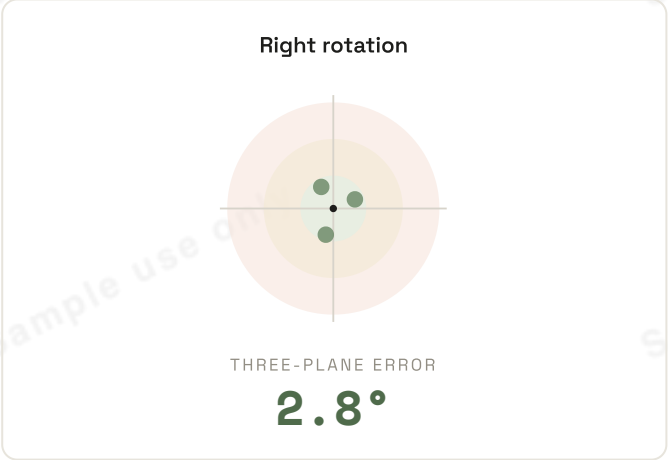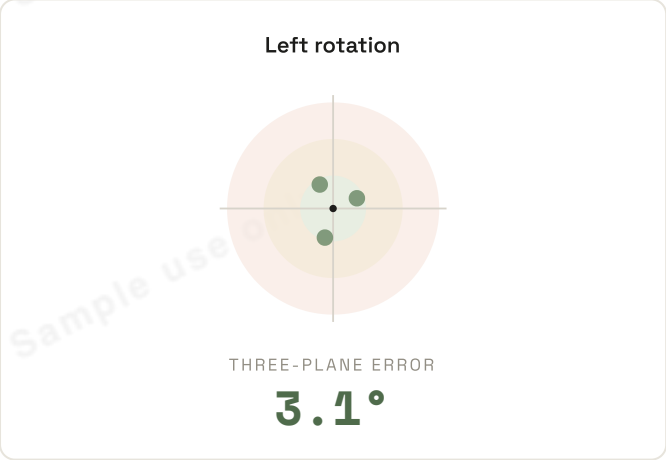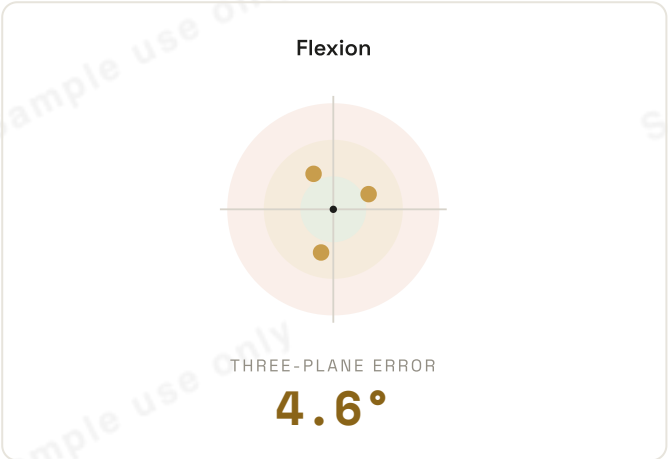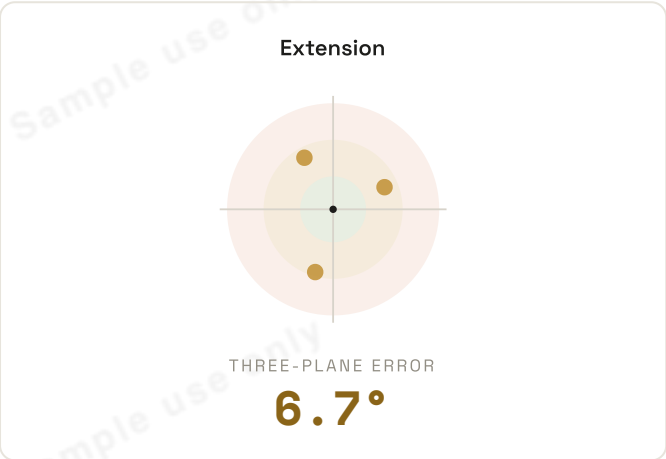

Each target shows the spread of return attempts around true neutral (centre). Tighter clusters mean better position sense. The value is the three-plane error.



NUMERICAL RESULTS

Joint position error — values

Three-plane error and its breakdown by plane, in degrees.

Extension			AVERAGE
THREE-PLANE ERROR			
6.7°			
FLEX / EXT	L / R ROT.	L / R LAT. FLEX.	
5.1°	2.6°	2.0°	

Flexion			AVERAGE
THREE-PLANE ERROR			
4.6°			
FLEX / EXT	L / R ROT.	L / R LAT. FLEX.	
3.7°	1.9°	0.9°	

Left rotation			AVERAGE
THREE-PLANE ERROR			
3.1°			
FLEX / EXT	L / R ROT.	L / R LAT. FLEX.	
1.9°	2.3°	0.5°	

Right rotation			AVERAGE
THREE-PLANE ERROR			
2.8°			
FLEX / EXT	L / R ROT.	L / R LAT. FLEX.	
1.0°	1.5°	1.7°	



OBJECTIVE · TARGET TRACKING

Sensorimotor control


64

SCORE

The patient follows a moving target (dotted) using head movement alone. The solid line is the path they traced. Deviation is the average drift from the target, in degrees, across three speeds.

Easy

IN RANGE

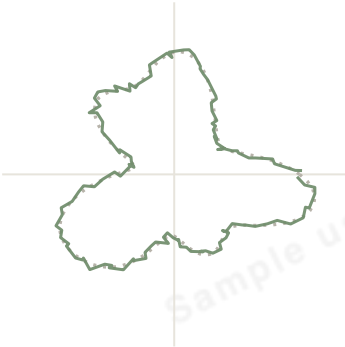

AVG. DEVIATION

0.7°


On target 79%

Behind 14%

Ahead 6%

Medium

MONITOR

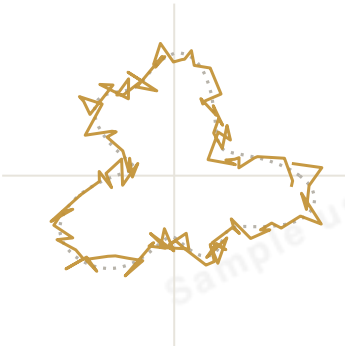

AVG. DEVIATION

1.5°


On target 45%

Behind 31%

Ahead 24%

Hard

● BELOW RANGE

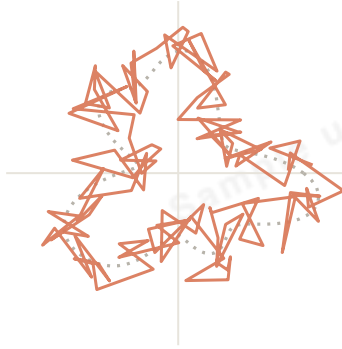

AVG. DEVIATION

2.7°

On target **22%**Behind **42%**Ahead **36%**

Control holds at slow speed and loosens as the target accelerates — the trace gets noisier and drifts further from the path. On-target / behind / ahead splits the time spent relative to the target.

DESKNECK · CERVICAL ASSESSMENT

SAMPLE USE ONLY · PATIENT SAMPLE 0001

METHOD

How we measure

Objective tools, scored against age norms, then re-tested to show change.

What gets measured

Movement, position sense, and control are captured objectively. Symptoms are self-reported. Nothing here rolls up into one number — each domain stands on its own and is read against people the same age.

Why re-test

A single result is a snapshot. The value is in the second one. We re-measure on the same tools, the same way, so any change is the patient's — not the method's.

Three ways forward

01 Discharge

Goals met. Work is done. This is a real outcome, not a loss.

02 Maintenance

Hold the gain. Lighter touch, checked at intervals.

03 Performance

Push past baseline toward a higher standard.

Sample document. This is an illustrative example of the DeskNeck assessment report format. The patient, identifier, and all values shown are fictional and for demonstration only. It is not a clinical record and describes no real person. DeskNeck makes no guarantee of any clinical result. Assessment is performed by Hugo Park, registered chiropractor (AHPRA CHI0002895435).